

Light efficiency:

92 Lumen/Watt

Light quality:

CRI: 91,6

Color temperature:

2609 K

Output: 117 lm

Peak: 430 cd

Power: 1,3 W

PF: 1,0



Product name:

PicoSpot³-927-LSST-350mA

Item number:

FLNP/PS1C/C01/0108/927/LSST/16558

Date and time:

10.07.2020 12:18:59

Description:

Toleranzen:

Lumen +/-4%

Candela +/-2,5%

Colour Temp +/-35 Grad K

CRI +/-0,7

Angular Resolution 1 Grad Step

Last Calibration 21.05.2021

Pruefer:


Peter Ulrich

Pruefort:

Lichtlabor


Gaustrasse13

55411 Bingen am Rhein

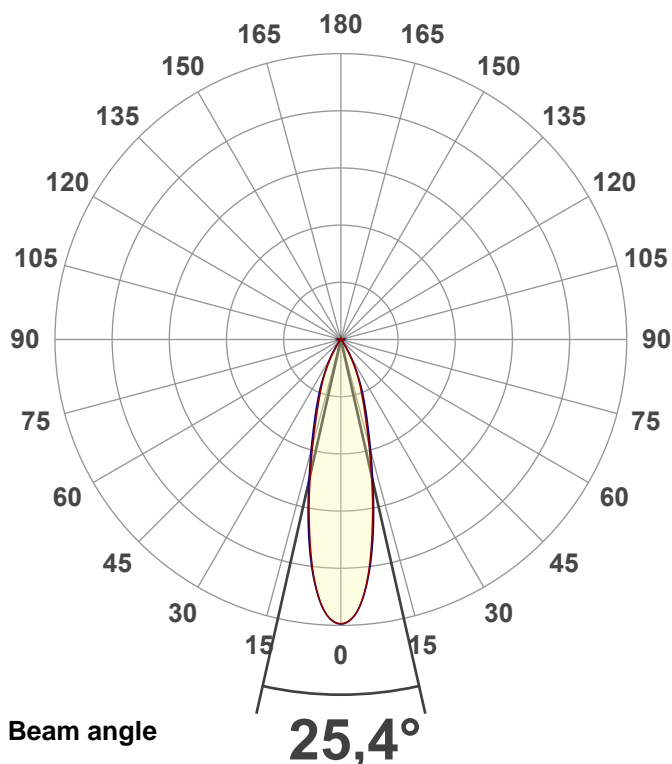



CIE 1931
x: 0,467
y: 0,410

Spectra

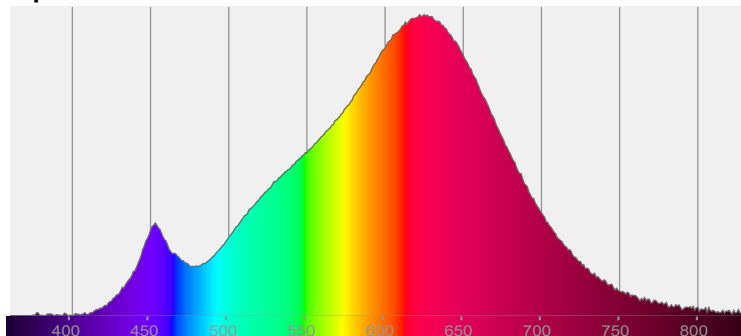


Power


Voltage: 3,65 V
Current: 0,350 A
Frequency: 0 Hz

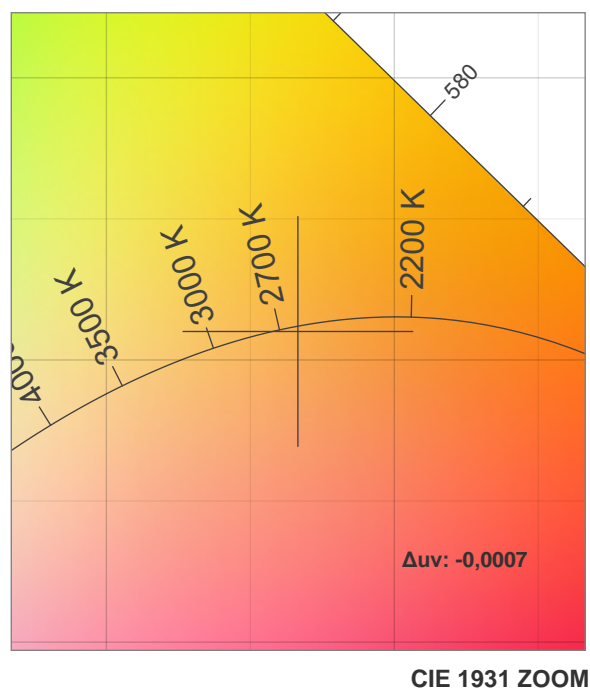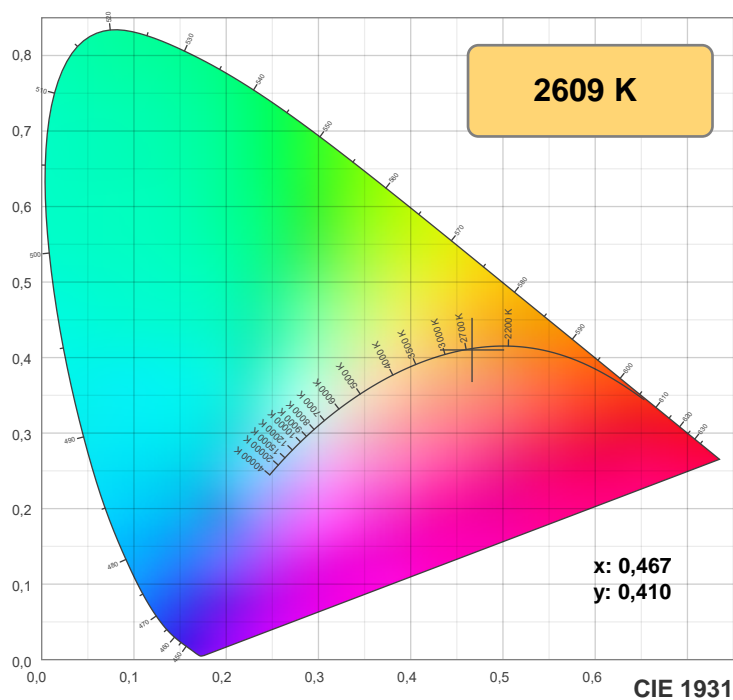

TM30: 91,1

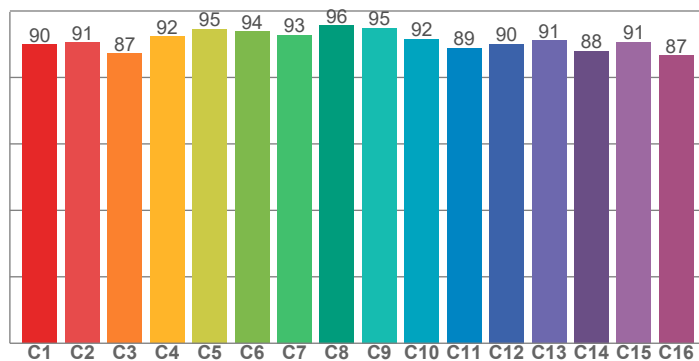

CRI: 91,6 (R1-R8)

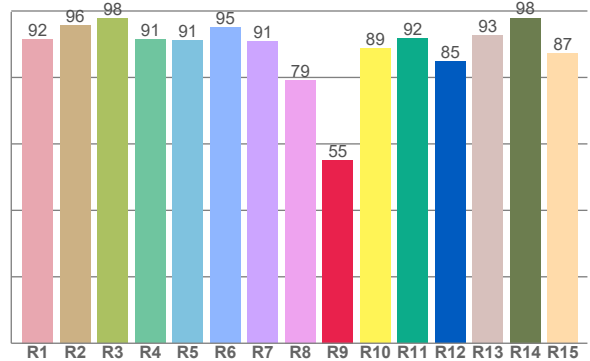

CRI R values, only R1-R8 are used to calculate final CRI value

R1	R2	R3	R4	R5	R6	R7	R8	R9	R10	R11	R12	R13	R14	R15
91,5	95,6	97,8	91,4	91,1	95,1	90,8	79,2	55,1	88,6	91,8	84,9	92,6	97,9	87,2


TM30 C values, 16 binned values out of total of 99 C values

C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
89,9	90,5	87,2	92,4	94,6	93,8	92,8	95,7	94,9	91,6	88,9	90,0	91,1	87,9	90,7	86,5

CQS Q values

Q1	Q2	Q3	Q4	Q5	Q6	Q7	Q8	Q9	Q10	Q11	Q12	Q13	Q14	Q15
85,8	94,5	87,8	87,3	89,6	89,1	87,7	89,3	96,1	91,7	90,7	89,9	90,0	84,8	84,8

CQS: 88,7

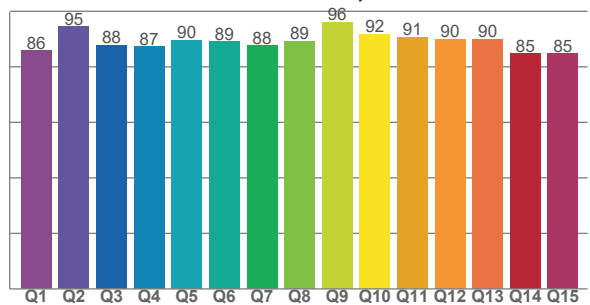

Color parameters

Color temperature	Color rendering index	Red component	Color fidelity	Color gamut	Color quality scale	Color coordinate cie 1931	Color coordinate cie 1931	Color coordinate	Color coordinate	Color deviation from black body
CCT	CRI	CRI R9	TM30 Rf	TM30 Rg	CQS	x	y	u	v	Δuv
2609 K	91,6	55,1	91,1	100,1	88,7	0,467	0,410	0,267	0,352	-0,0007







Rf 91,1


Fidelity index Rf

Rg 100,1

Gammut index Rg

Hue Bin	R _f	Graphic shifts (%)	
		Chroma	Hue
1	90	-6%	0%
2	91	-4%	4%
3	87	-1%	7%
4	92	1%	4%
5	95	3%	3%
6	94	4%	0%
7	93	1%	-4%
8	96	-1%	-2%
9	95	-3%	0%
10	92	-2%	5%
11	89	1%	7%
12	90	4%	2%
13	91	4%	-5%
14	88	4%	-9%
15	91	-1%	-6%
16	87	-4%	-10%

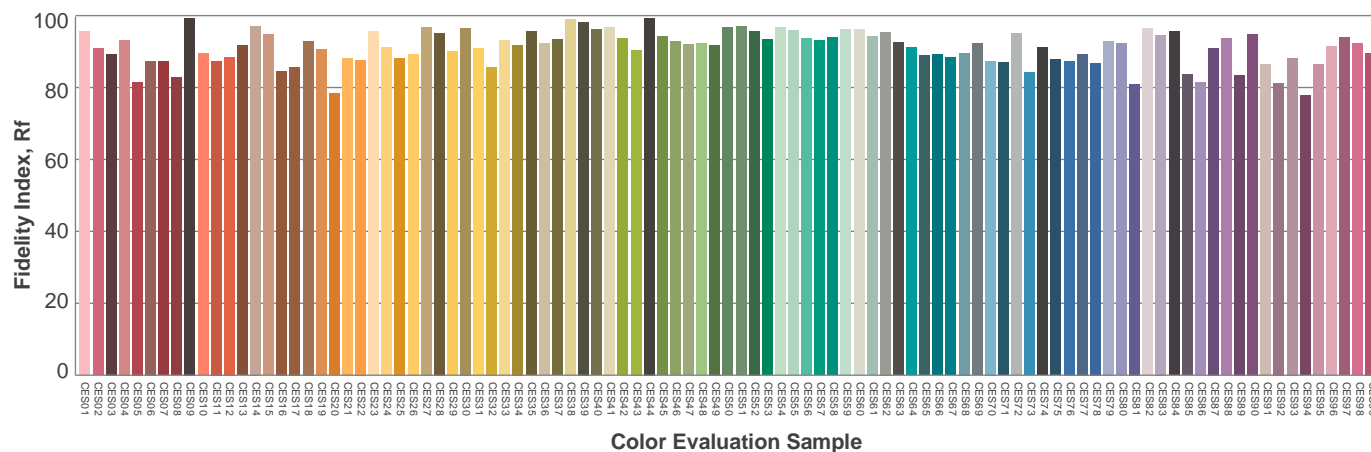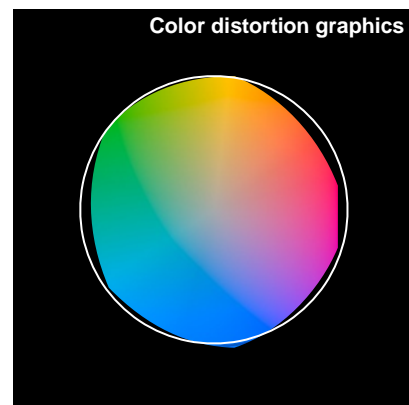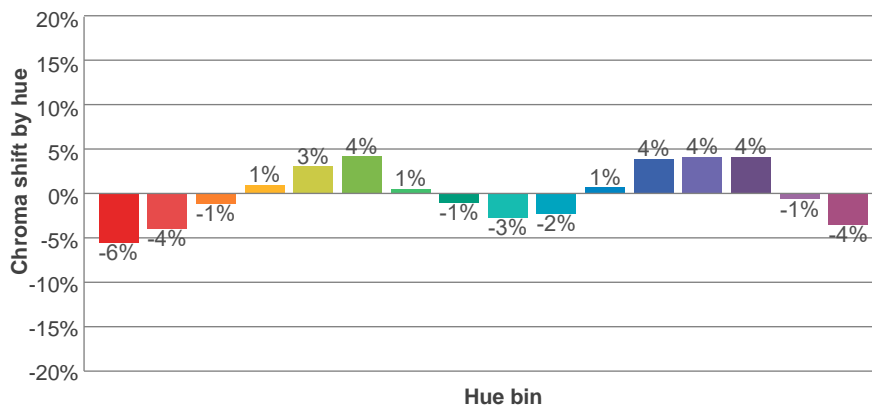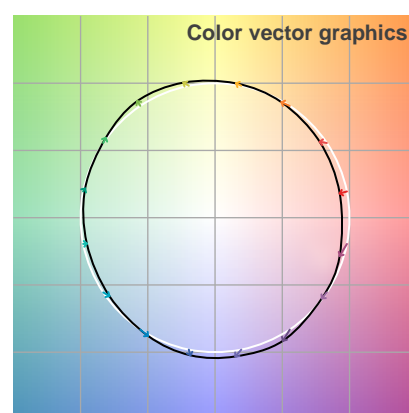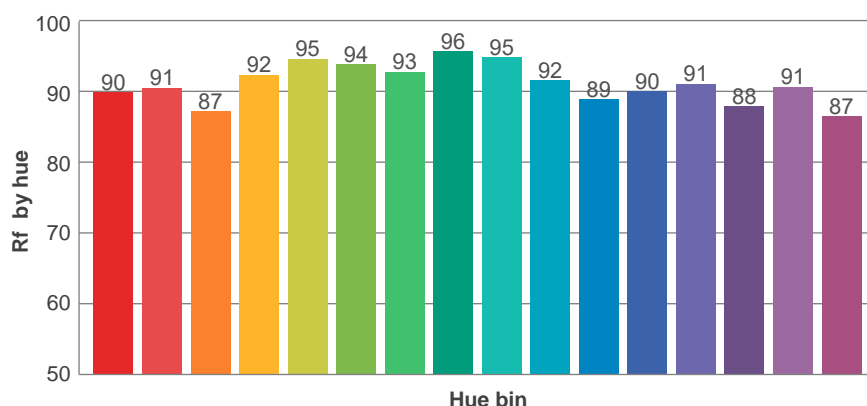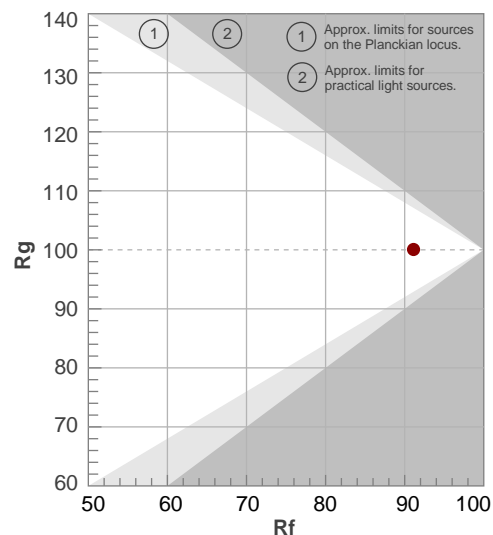

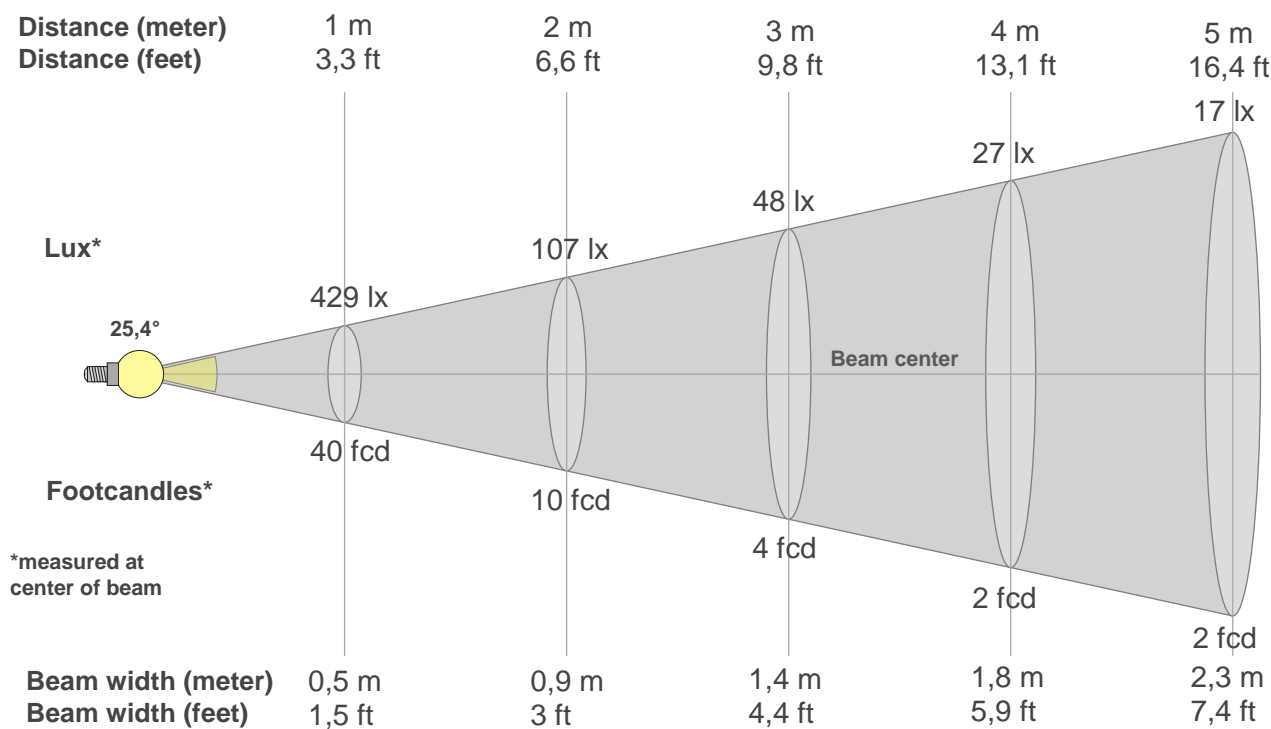

Beam intensities from 1-20m

1m	2m	3m	4m	5m	6m	7m	8m	9m	10m	11m	12m	13m	14m	15m	16m	17m	18m	19m	20m
3,3ft	6,6ft	9,8ft	13,1ft	16,4ft	19,7ft	23ft	26,2ft	29,5ft	32,8ft	36,1ft	39,4ft	42,7ft	45,9ft	49,2ft	52,5ft	55,8ft	59,1ft	62,3ft	65,6ft
429lx	107lx	48lx	27lx	17lx	12lx	9lx	7lx	5lx	4lx	4lx	3lx	3lx	2lx	2lx	2lx	1lx	1lx	1lx	1lx
39,9fcd	10fcd	4,4fcd	2,5fcd	1,6fcd	1,1fcd	0,8fcd	0,6fcd	0,5fcd	0,4fcd	0,3fcd	0,3fcd	0,2fcd	0,2fcd	0,2fcd	0,2fcd	0,1fcd	0,1fcd	0,1fcd	0,1fcd

Intensities in 0° c-plane

0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°
429	423	404	370	325	276	227	183	147	118	97	80	66	52	39	27	18	10	6	4
100%	99%	94%	86%	76%	64%	53%	43%	34%	27%	23%	19%	15%	12%	9%	6%	4%	2%	1%	1%

Intensities in 90° c-plane

0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°
429	422	403	372	330	283	235	192	157	129	106	88	70	54	40	30	21	13	8	5
100%	98%	94%	87%	77%	66%	55%	45%	37%	30%	25%	20%	16%	13%	9%	7%	5%	3%	2%	1%

Intensities in 180° c-plane


0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°
429	423	404	370	325	276	227	183	147	118	97	80	66	52	39	27	18	10	6	4
100%	99%	94%	86%	76%	64%	53%	43%	34%	27%	23%	19%	15%	12%	9%	6%	4%	2%	1%	1%

Intensities in 270° c-plane

0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°
429	422	403	372	330	283	235	192	157	129	106	88	70	54	40	30	21	13	8	5
100%	98%	94%	87%	77%	66%	55%	45%	37%	30%	25%	20%	16%	13%	9%	7%	5%	3%	2%	1%

Beam angle 50%	Field angle 10%	Cutoff angle 2,5%	Intensity ratio in 120° cone	Intensity ratio in 90° cone
25,4°	54,7°	68,5°	98,8%	97,9%

ISO candela diagram

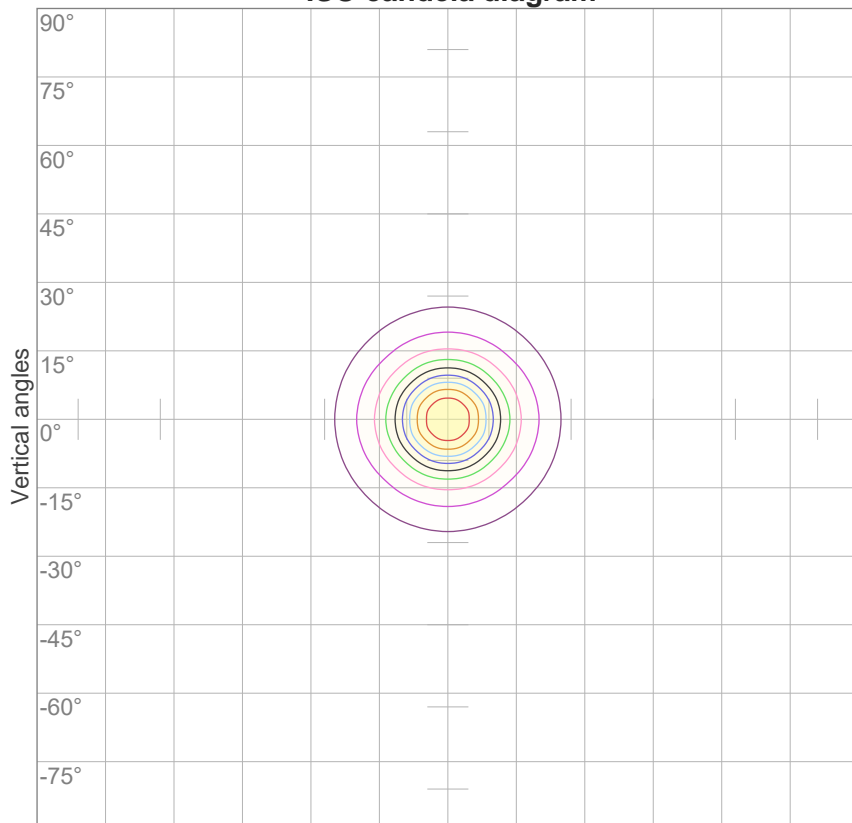


10%	43 cd
20%	86 cd
30%	129 cd
40%	172 cd
50%	215 cd
60%	257 cd
70%	300 cd
80%	343 cd
90%	386 cd

Conditions:

Number of c-planes: 16

Candela at center: 429 cd

ISO lux diagram

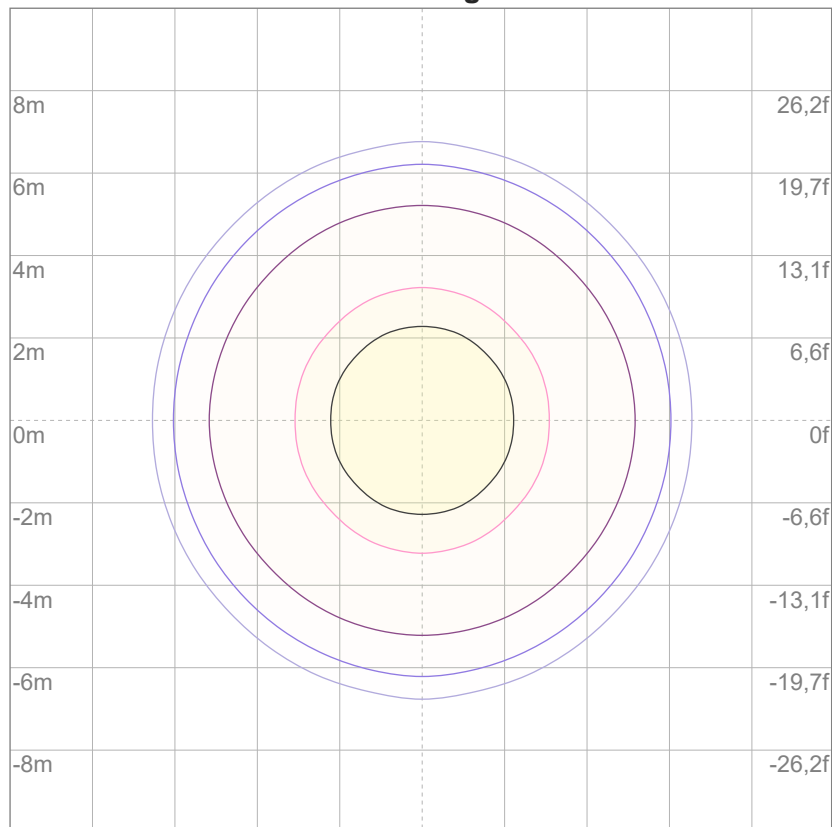

3%	0,129 lx
5%	0,215 lx
10%	0,429 lx
30%	1,29 lx
50%	2,15 lx

Conditions:

Number of c-planes: 16

Lux at center: 4,29 lx

*Lux distribution on a surface
when lamp is mounted at 10
meters from the surface.*

Glare Evaluation According to UGR


p Ceiling		70	70	50	50	30	70	70	50	50	30
p Walls		50	30	50	30	30	50	30	50	30	30
p Floor		20	20	20	20	20	20	20	20	20	20
Room size X Y		Viewing direction at right angles to lamp axis					Viewing direction parallel to lamp axis				
2H	2H	16,9	17,4	17,0	17,6	17,8	17,9	18,3	17,9	18,5	18,7
	3H	16,7	17,4	17,1	17,5	17,7	17,7	18,3	18,1	18,5	18,7
	4H	16,7	17,3	17,1	17,6	17,8	17,7	18,3	18,1	18,5	18,7
	6H	16,8	17,3	17,1	17,6	18,0	17,8	18,3	18,1	18,6	18,9
	8H	16,8	17,3	17,1	17,6	18,0	17,8	18,2	18,1	18,6	18,9
	12H	16,8	17,2	17,1	17,6	18,0	17,8	18,2	18,1	18,6	19,0
4H	2H	16,6	17,2	17,0	17,4	17,7	17,5	18,1	17,9	18,4	18,6
	3H	16,7	17,2	17,0	17,5	17,9	17,6	18,1	18,0	18,4	18,9
	4H	16,7	17,1	17,1	17,5	18,0	17,6	18,0	18,0	18,5	19,0
	6H	16,7	17,2	17,2	17,5	17,9	17,7	18,1	18,2	18,5	18,8
	8H	16,7	17,2	17,2	17,5	17,9	17,7	18,1	18,2	18,4	18,8
	12H	16,7	17,1	17,2	17,5	17,9	17,7	18,0	18,2	18,4	18,9
8H	4H	16,6	17,1	17,1	17,4	17,8	17,5	18,0	18,0	18,3	18,7
	6H	16,7	17,0	17,2	17,5	18,0	17,6	17,9	18,1	18,4	18,9
	8H	16,8	17,0	17,3	17,6	18,2	17,7	18,0	18,2	18,5	19,1
	12H	16,8	17,0	17,4	17,5	18,1	17,8	18,0	18,4	18,5	19,1
12H	4H	16,6	16,9	17,1	17,3	17,8	17,5	17,8	18,0	18,2	18,7
	6H	16,8	17,0	17,3	17,5	18,1	17,7	17,9	18,2	18,4	19,0
	8H	16,8	17,0	17,4	17,5	18,1	17,7	17,9	18,3	18,4	19,0
Variation of the observer position for the luminaire distance S											
S = 1.0H		5,6 / -4,2					5,7 / -4,4				
S = 1.5H		8,3 / -4,5					8,4 / -4,8				
S = 2.0H		10,2 / -5,0					10,4 / -5,0				
Standard table		n/a					n/a				
Correction summand		n/a					n/a				
Corrected glare indices referring to 117 lm total luminous flux											

Coefficients of Utilization

Ceiling reflectance	80				70				50			30			10			0
Wall reflectance	70	50	30	10	70	50	30	10	50	30	10	50	30	10	50	30	10	0
Floor reflectance	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	0
RCR	(RCR: Room Cavity Ratio) Room Values are expressed as percentage of Lumens delivered to the task surface																	
0	119	119	119	119	116	116	116	116	111	111	111	106	106	106	102	102	102	100
1	114	112	110	108	112	110	108	106	106	104	103	102	101	100	99	98	97	95
2	110	106	103	100	108	105	102	99	101	99	97	98	97	95	96	94	93	91
3	106	101	97	94	104	100	96	93	97	94	92	95	92	90	93	91	89	88
4	102	97	92	89	101	95	91	88	93	90	87	92	89	86	90	87	85	84
5	99	92	88	85	98	92	87	84	90	86	83	88	85	83	87	84	82	81
6	96	89	84	81	94	88	84	81	87	83	80	85	82	80	84	81	79	78
7	93	85	81	78	91	85	80	77	84	80	77	83	79	77	82	78	76	75
8	90	82	78	75	89	82	77	74	81	77	74	80	76	74	79	76	74	72
9	87	79	75	72	86	79	75	72	78	74	72	77	74	71	77	73	71	70
10	84	77	72	69	83	76	72	69	76	72	69	75	71	69	74	71	69	68

LAMPS (number of lamps)


Luminaire budgetary diagram

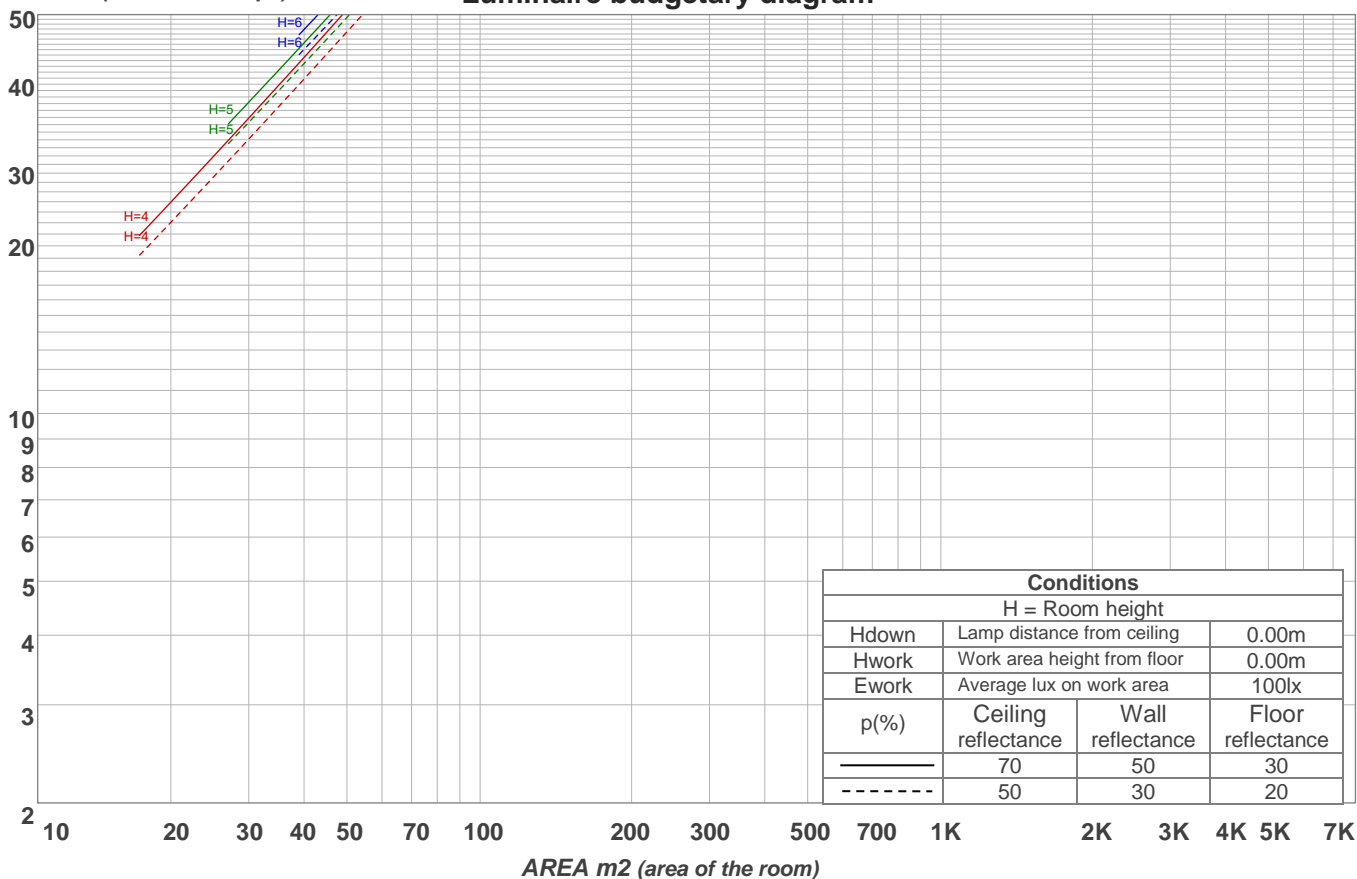

Zonal Lumen Summary

0°-10°	10°-20°	20°-30°	30°-40°	40°-50°	50°-60°	60°-70°	70°-80°	80°-90°
33,6 lm	47,0 lm	27,0 lm	6,64 lm	1,09 lm	0,686 lm	0,514 lm	0,410 lm	0,237 lm
90°-100°	100°-110°	110°-120°	120°-130°	130°-140°	140°-150°	150°-160°	160°-170°	170°-180°
0,089 lm	0,044 lm	0,023 lm	0,020 lm	0,017 lm	0,014 lm	0,010 lm	0,006 lm	0,002 lm

Warmup curve

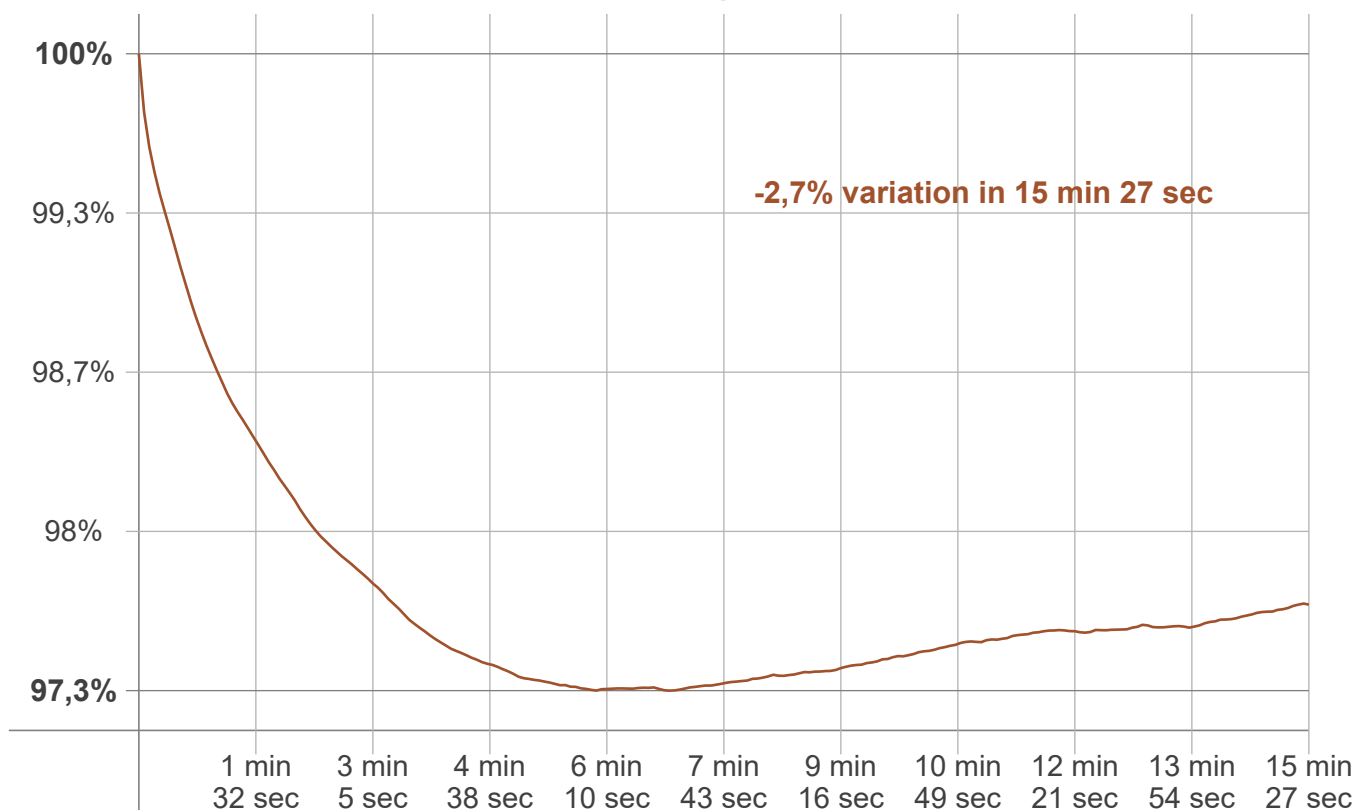

Warmup result

Warmup time:	Lamp stabilized in 15 min 27 sec
Warmup variation	-2,7%

Warmup conditions

Stable period:	15 min
Stable change max:	2,0%
Minimum time:	15 min

Color temperature change

CCT start	CCT change	CCT end
2619 K	-10 K	2609 K

Output change

Output start	Output change	Output end
119 lm	-2 lm	117 lm